



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Sirolan Laserscan Micron Test Report

Verein Österreichischer Alpakazüchter/Alpaka Assn. Austria
Stainach-pürgg
4844 Linz, Regau Austria

10/06/16

Test No: 935551


Animal and Sample Description

Animal Name: Salvatore (Alpaka-Valley)
Breed: Alpaca(Huacaya)
Sex: XXXXX
Color: XXXXX

Animal ID: XXXXX
Sample Location: Side
Sample Date: 05/15/16
Age: XXXXX

Laboratory Data

Mean Fiber Diameter: 17.1 microns
Standard Deviation: 3.6 microns
Coefficient of Variation: 20.9 %
Fibers Greater Than 30 microns: 1.0 %

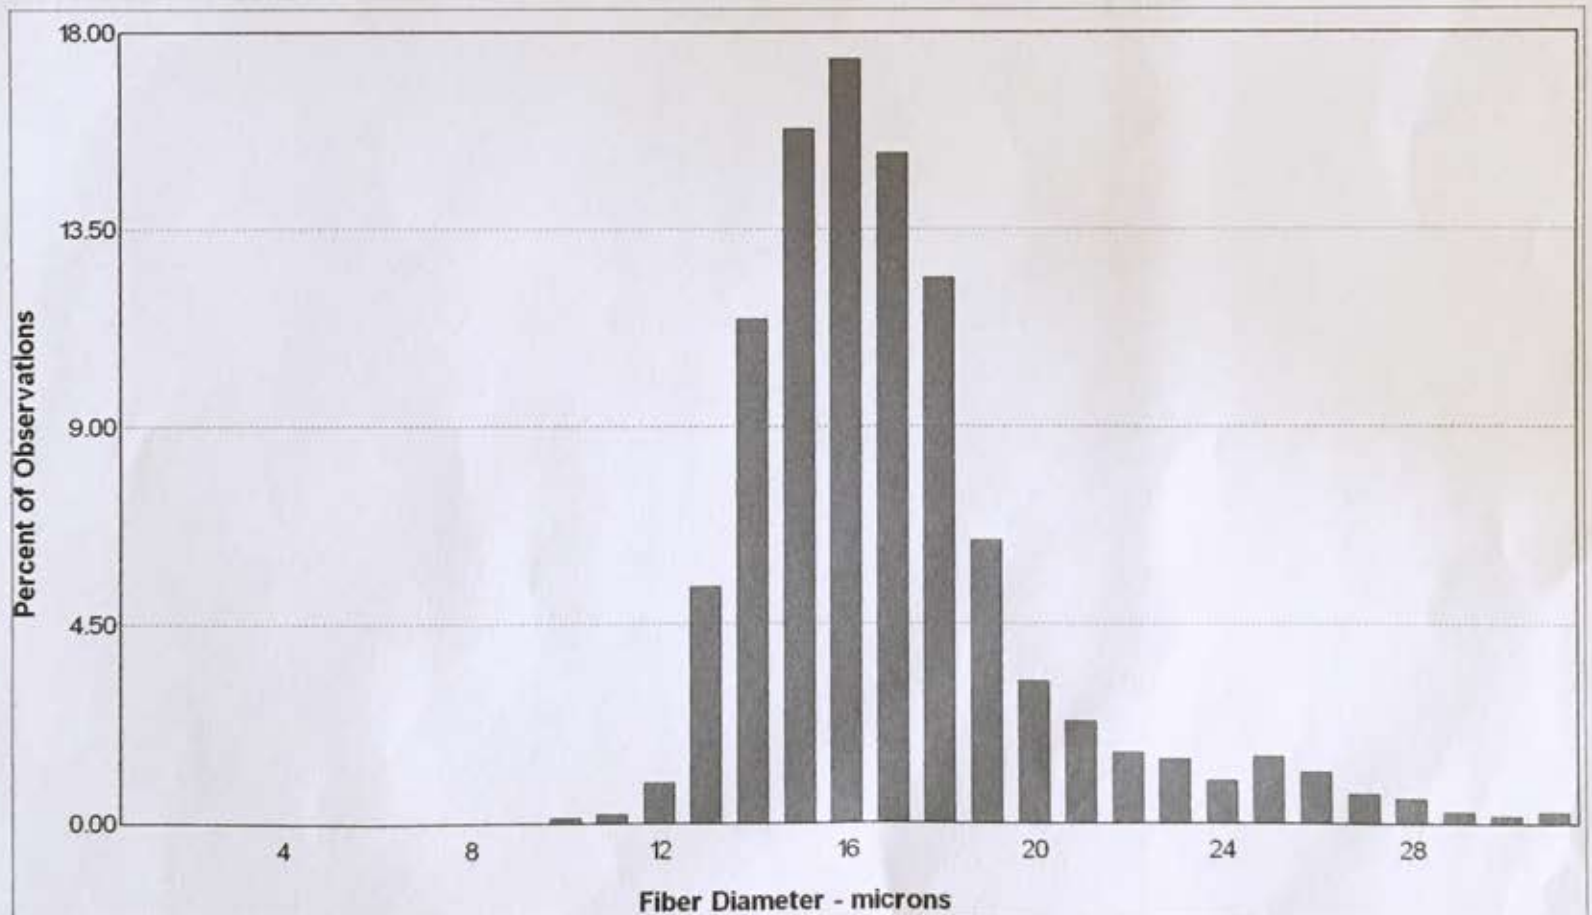

This Test Performed According to I.W.T.O Method 12